

‘The Forceshoe’: What has been achieved?

Ambulatory estimation of ankle and foot dynamics and center of mass movement

H. Martin Schepers¹, Bart F.J.M Koopman¹, Edwin H.F. van Asseldonk¹, Jaap H. Buurke², Peter H. Veltink¹

¹Institute for BioMedical Technology (BMTI), University of Twente, Enschede, The Netherlands

²Roessingh Research and Development (RRD), Enschede, The Netherlands

h.m.schepers@ewi.utwente.nl

Abstract—Gait analysis is commonly done in gait laboratories, where several gait variables are estimated using measurement systems installed in the laboratory. The major drawback of these measurement systems is their restriction to the laboratory. This study shows the possibilities of an ambulatory measurement system: the forceshoe. The forceshoe consists of an orthopaedic sandal with force/moment sensors and inertial sensors attached to the heel and the forefoot. Ankle and foot dynamics as well as center of mass movement have been estimated. Moreover, the ambulatory system has been compared to a reference system consisting of an optical position measurement system and two force plates.

Keywords—ground reaction force; center of mass; dynamics; ambulatory

1. INTRODUCTION

Traditionally, human body movement analysis is done in so-called ‘gait laboratories’, equipped with several measurement systems such as optical position measurement systems, EMG or force plates. The measured signals are used to estimate important gait variables. An important variable is the center of mass, an imaginary point at which the total body mass can be assumed to be concentrated. Several methods exist for center of mass estimation, of which the segmental kinematics method and the double integration of ground reaction force method are the most important ones. Other important variables are joint moment and powers. These can be estimated from estimations of body movement and ground reaction forces by applying inverse dynamics methods.

A major drawback of the existing systems is the restriction to the laboratory environment. Therefore research is required for the development of measurement systems to perform these measurements in an ambulatory environment.



Figure 1. Picture of the forceshoe with two force/moment sensors beneath the heel and the forefoot and two inertial sensors rigidly attached to the force/moment sensors.

The objective of this study is to give an overview of the possibilities of the forceshoe. The forceshoe is an ambulatory measurement system able to measure the ground reaction force and movement of foot and ankle.

2. METHODS

The forceshoe consists of an orthopaedic sandal equipped with two six-degrees-of-freedom force/moment sensors beneath the heel and the forefoot. Moreover, an inertial sensor is rigidly attached to each force/moment sensor (Fig. 1).

Estimation of Ankle and Foot Dynamics

The estimation of ankle and foot dynamics requires the ground reaction force and movement of foot and ankle to be determined. The ground reaction force is measured by the force/moment sensors beneath the sole of the forceshoe. The movement of foot and ankle is estimated from signals measured by the inertial sensors (Xsens, MTx) connected to the force/moment sensors. A detailed description of the measurement system and methods can be found in [1].

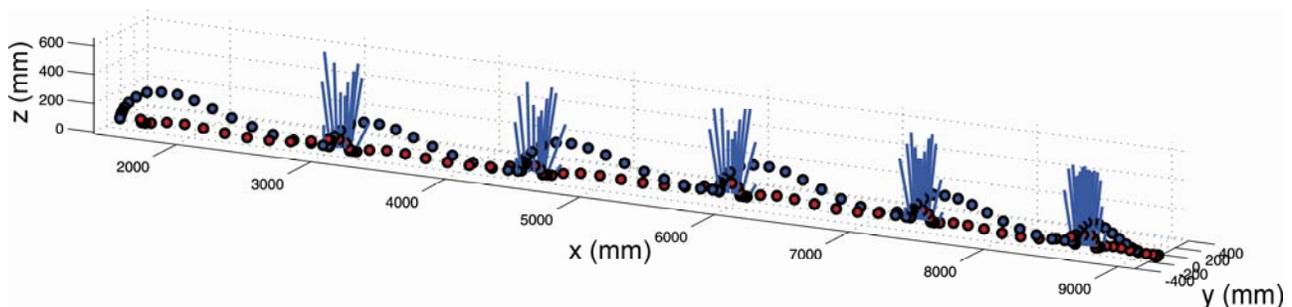


Figure 2. Estimation of the ground reaction force (blue lines) and the movement of heel (blue dots) and forefoot (red dots) of the right foot during several steps.

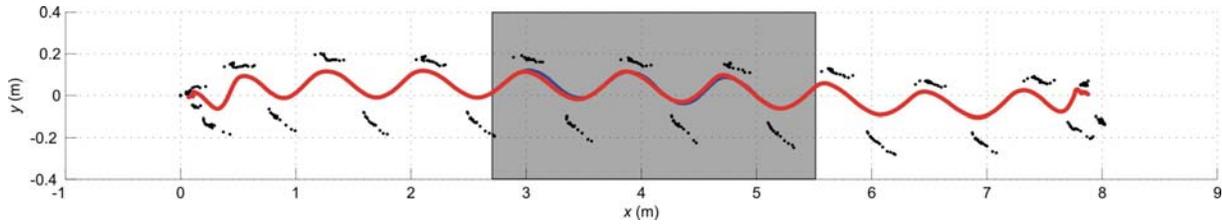


Figure 3. Estimated center of mass by the ambulatory (red) and reference (blue) systems. The center of pressure is indicated by the black dots on either side of the center of mass, where each dot represents a time sample. Moreover, the measurement volume of the reference system is indicated by the gray area.

Estimation of Center of Mass Movement

The estimation of center of mass movement is based on fusion of center of pressure data with double integrated ground reaction force data, both estimated from signals measured by the forcesshoe. The fusion is based on a frequency domain method, which is described in [2].

Experimental Methods

Several measurements were performed with the forcesshoe. During the measurements, a subject was asked to walk through the gait laboratory while wearing the forcesshoe. The accuracy of the ambulatory system was validated by comparing it to a reference system consisting of an optical measurement system and two force plates.

3. RESULTS

An estimation of the ground reaction force is shown in Fig. 4. The signals measured with the forcesshoe show good correspondence with the signals measured with the force plate, which is confirmed by the rms difference between the magnitudes of the ground reaction force, being 0.02 N/N or 1.8 % of the maximal magnitude.

Fig. 2 shows an integration of the measured ground reaction force with the estimated position of the heel and forefoot sensor. The figure indicates the possibility of the ambulatory measurement system to measure several steps during a single measurement, which is not possible with the reference system. This is also shown in Fig. 3, which shows the estimated center

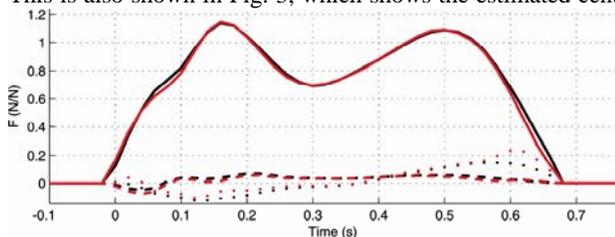


Figure 4. Three components of the ground reaction force as a function of time estimated by the ambulatory (red) and reference (black) systems (forward: dotted, lateral: dashed, vertical solid).

of mass movement estimated by the ambulatory (red) and reference (blue) systems. On either side of the center of mass, the center of pressure is indicated by the black dots where each dot represents a time sample. The rms difference between the magnitudes of the center of mass displacement estimated by the ambulatory and the reference measurement systems was 0.025 ± 0.007 m.

4. DISCUSSION

This study has shown the possibilities of the forcesshoe for ambulatory measurements. Ankle and foot dynamics as well as the movement of the center of mass were estimated and the accuracy was validated using a reference measurement system. A more detailed evaluation with respect to the performance of the forcesshoe can be found in [1,2]. Overall, the accuracy of the results obtained with the ambulatory measurement system was comparable to other studies described in literature [3,4].

5. ACKNOWLEDGMENT

The financial support from the Dutch Ministry of Economic Affairs for the FreeMotion project is gratefully acknowledged.

6. REFERENCES

- [1] H.M. Schepers, H.F.J.M. Koopman, P.H. Veltink, Ambulatory assessment of ankle and foot dynamics, IEEE Trans. Biomed. Eng, 54(5): pp. 895-902, 2007.
- [2] H.M. Schepers, E.H.F. van Asseldonk, J.H. Buurke, P.H. Veltink, Ambulatory estimation of center of mass displacement during walking, unpublished.
- [3] B.A. MacWilliams, M. Cowley, D.E. Nicholson, Foot kinematics and kinetics during adolescent gait, Gait Posture, 17(3): pp. 214-224, 2003.
- [4] M.H.A. Eames, A. Cosgrove, R. Baker, Comparing methods of estimating the total body centre of mass in three-dimensions in normal and pathological gaits, Hum Mov Sci, 18(5): pp. 637-646, 1999.